



UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

APPLICATION NO.	FILING DATE	FIRST NAMED INVENTOR	ATTORNEY DOCKET NO.	CONFIRMATION NO.
10/773,631	02/06/2004	Alexander Star	612407-23	8346
23879	7590	11/01/2006		
BRIAN M BERLINER, ESQ O'MELVENY & MYERS, LLP 400 SOUTH HOPE STREET LOS ANGELES, CA 90071-2899			EXAMINER SINES, BRIAN J	
			ART UNIT	PAPER NUMBER
			1743	

DATE MAILED: 11/01/2006

Please find below and/or attached an Office communication concerning this application or proceeding.

Office Action Summary

Application No.

10/773,631

Applicant(s)

STAR ET AL.

Examiner

Brian J. Sines

Art Unit

1743

-- The MAILING DATE of this communication appears on the cover sheet with the correspondence address --

Period for Reply

A SHORTENED STATUTORY PERIOD FOR REPLY IS SET TO EXPIRE 3 MONTH(S) OR THIRTY (30) DAYS, WHICHEVER IS LONGER, FROM THE MAILING DATE OF THIS COMMUNICATION.

- Extensions of time may be available under the provisions of 37 CFR 1.136(a). In no event, however, may a reply be timely filed after SIX (6) MONTHS from the mailing date of this communication.
- If NO period for reply is specified above, the maximum statutory period will apply and will expire SIX (6) MONTHS from the mailing date of this communication.
- Failure to reply within the set or extended period for reply will, by statute, cause the application to become ABANDONED (35 U.S.C. § 133). Any reply received by the Office later than three months after the mailing date of this communication, even if timely filed, may reduce any earned patent term adjustment. See 37 CFR 1.704(b).

Status

- 1) ☒ Responsive to communication(s) filed on 07 August 2006.
- 2a) ☒ This action is **FINAL**. 2b) ☐ This action is non-final.
- 3) ☐ Since this application is in condition for allowance except for formal matters, prosecution as to the merits is closed in accordance with the practice under *Ex parte Quayle*, 1935 C.D. 11, 453 O.G. 213.

Disposition of Claims

- 4) ☒ Claim(s) 1-21 is/are pending in the application.
- 4a) Of the above claim(s) 6-19 is/are withdrawn from consideration.
- 5) ☐ Claim(s) _____ is/are allowed.
- 6) ☒ Claim(s) 1-5, 20 and 21 is/are rejected.
- 7) ☐ Claim(s) _____ is/are objected to.
- 8) ☐ Claim(s) _____ are subject to restriction and/or election requirement.

Application Papers

- 9) ☐ The specification is objected to by the Examiner.
- 10) ☒ The drawing(s) filed on 2/6/2004 is/are: a) ☐ accepted or b) ☒ objected to by the Examiner.
Applicant may not request that any objection to the drawing(s) be held in abeyance. See 37 CFR 1.85(a).
Replacement drawing sheet(s) including the correction is required if the drawing(s) is objected to. See 37 CFR 1.121(d).
- 11) ☐ The oath or declaration is objected to by the Examiner. Note the attached Office Action or form PTO-152.

Priority under 35 U.S.C. § 119

- 12) ☐ Acknowledgment is made of a claim for foreign priority under 35 U.S.C. § 119(a)-(d) or (f).
- a) ☐ All b) ☐ Some * c) ☐ None of:
1. ☐ Certified copies of the priority documents have been received.
 2. ☐ Certified copies of the priority documents have been received in Application No. _____.
 3. ☐ Copies of the certified copies of the priority documents have been received in this National Stage application from the International Bureau (PCT Rule 17.2(a)).
- * See the attached detailed Office action for a list of the certified copies not received.

Attachment(s)

- | | |
|--|---|
| 1) <input checked="" type="checkbox"/> Notice of References Cited (PTO-892) | 4) <input type="checkbox"/> Interview Summary (PTO-413)
Paper No(s)/Mail Date. _____ |
| 2) <input type="checkbox"/> Notice of Draftsperson's Patent Drawing Review (PTO-948) | 5) <input type="checkbox"/> Notice of Informal Patent Application |
| 3) <input type="checkbox"/> Information Disclosure Statement(s) (PTO/SB/08)
Paper No(s)/Mail Date _____ | 6) <input type="checkbox"/> Other: _____ |

DETAILED ACTION***Drawings***

The drawings are objected to under 37 CFR 1.83(a). The drawings must show every feature of the invention specified in the claims. Therefore, the sample exposure portion and the gate electrode of the sensing device must be clearly shown and labeled or the feature(s) canceled from the claim(s). No new matter should be entered.

Corrected drawing sheets in compliance with 37 CFR 1.121(d) are required in reply to the Office action to avoid abandonment of the application. Any amended replacement drawing sheet should include all of the figures appearing on the immediate prior version of the sheet, even if only one figure is being amended. The figure or figure number of an amended drawing should not be labeled as "amended." If a drawing figure is to be canceled, the appropriate figure must be removed from the replacement sheet, and where necessary, the remaining figures must be renumbered and appropriate changes made to the brief description of the several views of the drawings for consistency. Additional replacement sheets may be necessary to show the renumbering of the remaining figures. Each drawing sheet submitted after the filing date of an application must be labeled in the top margin as either "Replacement Sheet" or "New Sheet" pursuant to 37 CFR 1.121(d). If the changes are not accepted by the examiner, the applicant will be notified and informed of any required corrective action in the next Office action. The objection to the drawings will not be held in abeyance.

Claim Rejections - 35 USC § 112

The following is a quotation of the second paragraph of 35 U.S.C. 112:

The specification shall conclude with one or more claims particularly pointing out and distinctly claiming the subject matter which the applicant regards as his invention.

Art Unit: 1743

Claims 20 and 21 are rejected under 35 U.S.C. 112, second paragraph, as being indefinite for failing to particularly point out and distinctly claim the subject matter which applicant regards as the invention.

Claims 20 and 21 are rejected under 35 U.S.C. 112, second paragraph, as being incomplete for omitting essential structural cooperative relationships of elements, such omission amounting to a gap between the necessary structural connections. See MPEP § 2172.01. The omitted structural cooperative relationships are: Regarding claim 21, the claim merely recites the incorporation of a gate electrode with the claimed device. It is unclear as to how the gate electrode is connected with the recited device components (e.g., the nanotube, electrical contact and sample exposure portion). Is the gate electrode in electrical communication with the nanotube or sample exposure portion? The structure which goes to make up the device must be clearly and positively specified. The structure must be organized and correlated in such a manner as to present a complete operative device.

Claim Rejections - 35 USC § 103

The following is a quotation of 35 U.S.C. 103(a) which forms the basis for all obviousness rejections set forth in this Office action:

(a) A patent may not be obtained though the invention is not identically disclosed or described as set forth in section 102 of this title, if the differences between the subject matter sought to be patented and the prior art are such that the subject matter as a whole would have been obvious at the time the invention was made to a person having ordinary skill in the art to which said subject matter pertains. Patentability shall not be negated by the manner in which the invention was made.

The factual inquiries set forth in *Graham v. John Deere Co.*, 383 U.S. 1, 148 USPQ 459 (1966), that are applied for establishing a background for determining obviousness under 35 U.S.C. 103(a) are summarized as follows:

1. Determining the scope and contents of the prior art.


Art Unit: 1743


2. Ascertaining the differences between the prior art and the claims at issue.
3. Resolving the level of ordinary skill in the pertinent art.
4. Considering objective evidence present in the application indicating obviousness or nonobviousness.

Claims rejected under 35 U.S.C. 103(a) as being unpatentable over Dai et al. (U.S. Pat. No. 6,528,020 B1) (hereinafter "Dai") in view of Akioka et al. (U.S. Pat. No. 6,464,940 B1) (hereinafter "Akioka").


Regarding claims 1 and 2, Dai teaches an apparatus comprising: a substrate 22, 30; at least one nanotube 20, 32 disposed on the substrate; at least one electrical contact 23, 33, wherein the contact is in electrical communication with the at least one nanotube (see figures 2 and 3B; col. 4, lines 23 – 65).

The use of the recited liquid with the sensing device during operation is considered a statement of intended use and is not considered a positively recited structural limitation of the device. The manner of operating an apparatus does not differentiate an apparatus claim from the prior art, if the prior art apparatus teaches all of the structural limitations of the claim. Furthermore, apparatus claims must be structurally distinguishable from the prior art in terms of structure, not function (see MPEP § 2114).

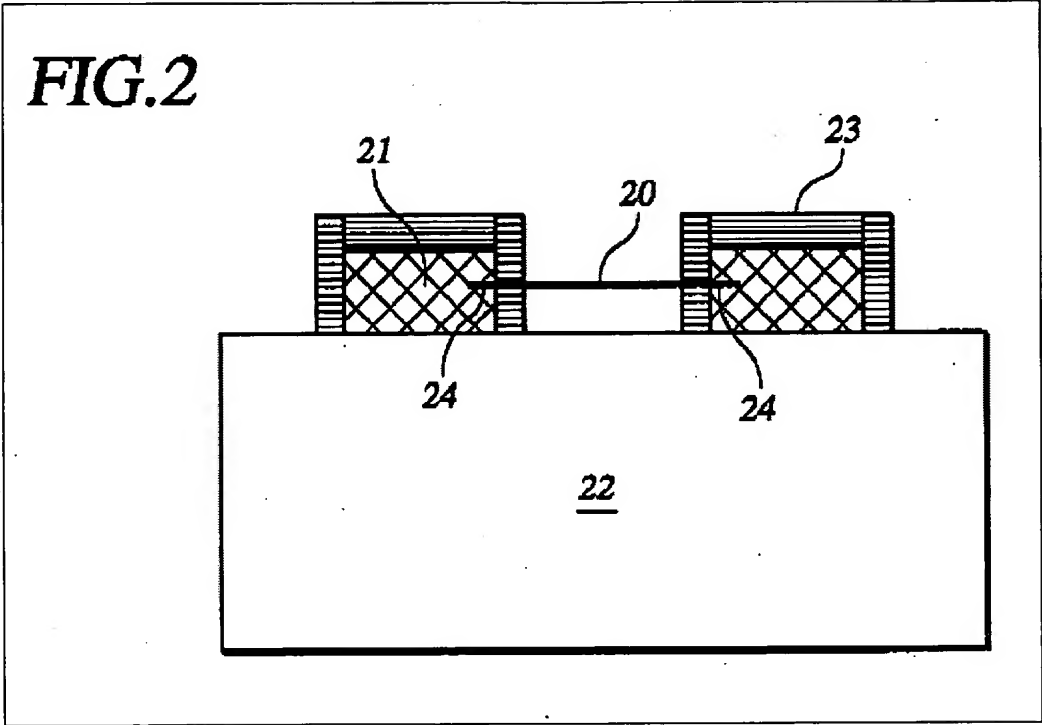

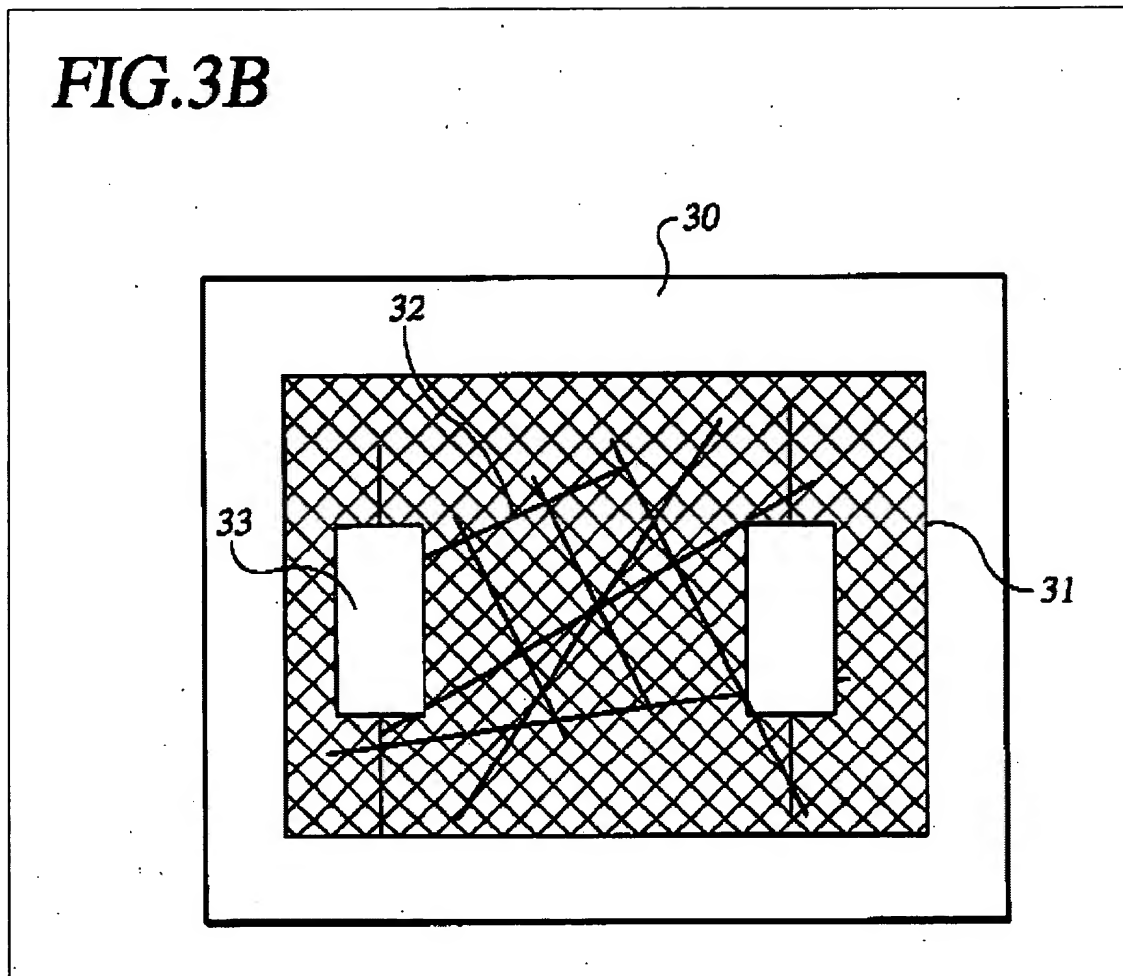

Dai does not specifically teach the incorporation of a sample exposure portion to maintain a liquid analyte sample in contact with at least one nanotube. However, the use of containing means for holding a sample for analysis with sensing devices is considered well known in the art (see MPEP §2144.03). For example, Akioka teaches a sensing device comprising a sample exposure portion (e.g., storage part 110) with electrical contact 107 for sensing the solution 105 (see, e.g., col. 2, lines 15 – 28; figure 1).

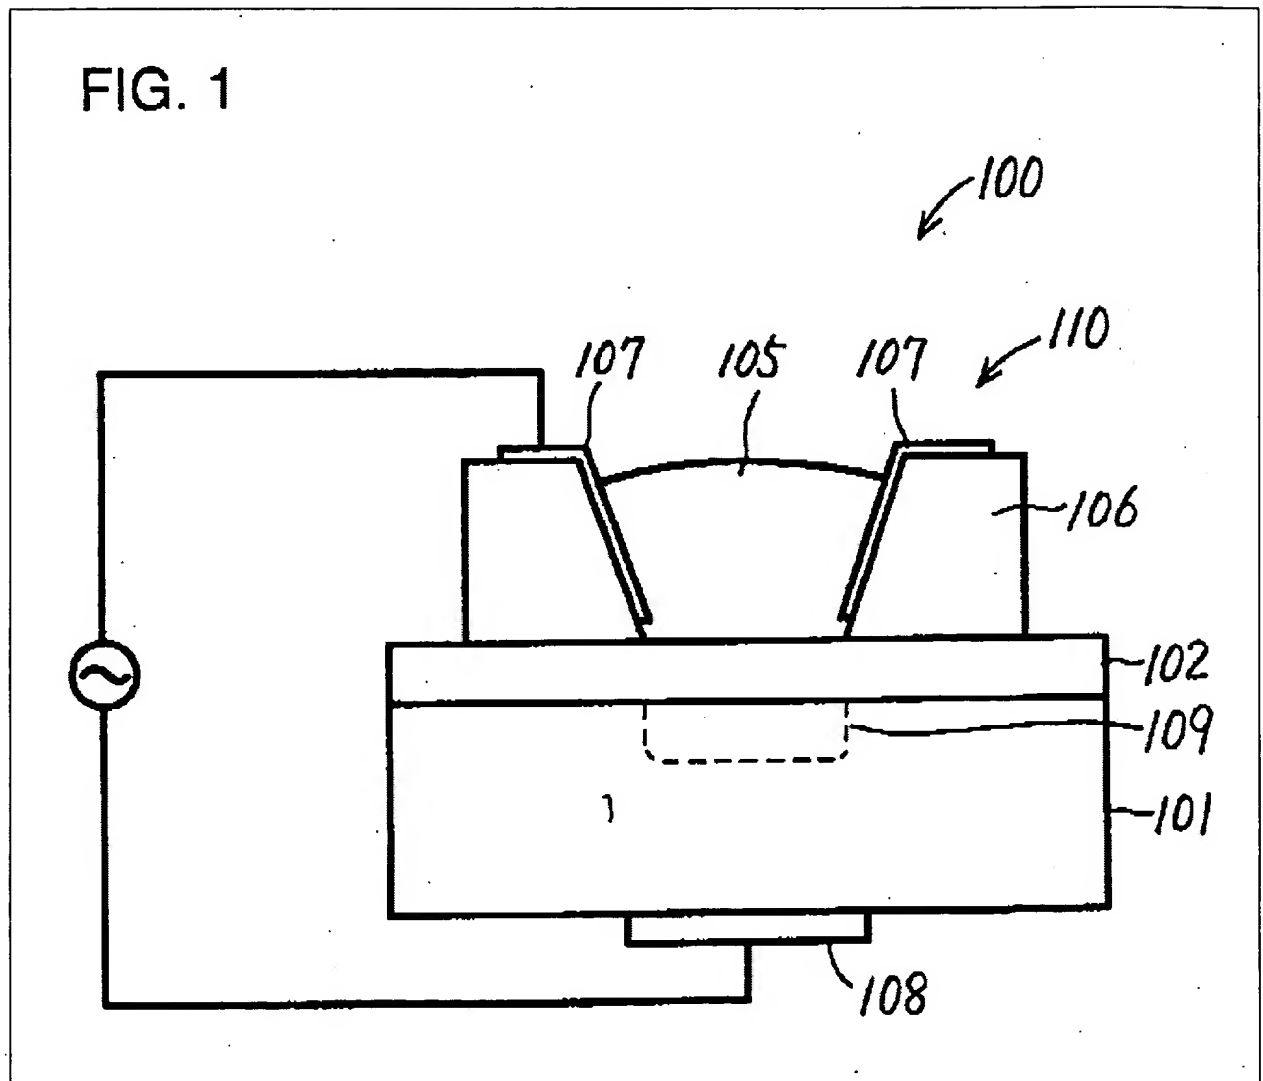

Hence, as indicated by Akioka, a person of ordinary skill in the art would accordingly have had a reasonable expectation for success of incorporating such a sample exposure means with a sensing device for analyzing a sample solution (see MPEP § 2143.02). Therefore, it would have been obvious to a person of ordinary skill in the art to incorporate a sample exposure portion as claimed with the disclosed sensing device to facilitate effective liquid analyte sample contact with the nanotube for sensing.

Art Unit: 1743

Regarding claim 3, as shown in figures 2 and 3B, the nanotube 20, 32 spans the distance between two electrical contacts 23, 33.

Regarding claim 4, the contacts 23, 33 comprises titanium (see col. 4, lines 23 – 65).

Regarding claim 5, the substrate comprises a silicon material (see col. 11 – 16).

Response to Arguments

Applicant's arguments with respect to the present claims have been considered but are moot in view of the new ground(s) of rejection.

Conclusion

Applicant's amendment necessitated the new ground(s) of rejection presented in this Office action. Accordingly, **THIS ACTION IS MADE FINAL**. See MPEP § 706.07(a).

Applicant is reminded of the extension of time policy as set forth in 37 CFR 1.136(a).

A shortened statutory period for reply to this final action is set to expire **THREE MONTHS** from the mailing date of this action. In the event a first reply is filed within **TWO MONTHS** of the mailing date of this final action and the advisory action is not mailed until after the end of the **THREE-MONTH** shortened statutory period, then the shortened statutory period will expire on the date the advisory action is mailed, and any extension fee pursuant to 37 CFR 1.136(a) will be calculated from the mailing date of the advisory action. In no event, however, will the statutory period for reply expire later than **SIX MONTHS** from the date of this final action.

Any inquiry concerning this communication or earlier communications from the examiner should be directed to Brian J. Sines, whose telephone number is (571) 272-1263. The examiner can normally be reached on Monday - Friday (11 AM - 8 PM EST).

Art Unit: 1743

If attempts to reach the examiner by telephone are unsuccessful, the examiner's supervisor, Jill A. Warden can be reached on (571) 272-1267. The fax phone number for the organization where this application or proceeding is assigned is 571-273-8300.

Information regarding the status of an application may be obtained from the Patent Application Information Retrieval (PAIR) system. Status information for published applications may be obtained from either Private PAIR or Public PAIR. Status information for unpublished applications is available through Private PAIR only. For more information about the PAIR system, see <http://pair-direct.uspto.gov>. Should you have questions on access to the Private PAIR system, contact the Electronic Business Center (EBC) at 866-217-9197 (toll-free).

A handwritten signature in black ink, appearing to read "Brian Sine". The signature is written in a cursive, flowing style with a large initial "B" and a long, sweeping underline.